


Alert Symbols The safety notices associated with the following should be given special attention when they appear in maintenance, operating and emergency procedures in the guide.

-  CAUTION indicates that a particular procedure or precaution must be followed to avoid system irregularity or possible damage to the product.
-  NOTE indicates special information to improve the ease of maintaining the product, or to clarify important information.
-  WARNING indicates that the personal safety of the patient, end user or technician could be compromised by disregarding the WARNING. Not following instructions may result in an injury.



 NOTE: System will deflate when unit is turned OFF.

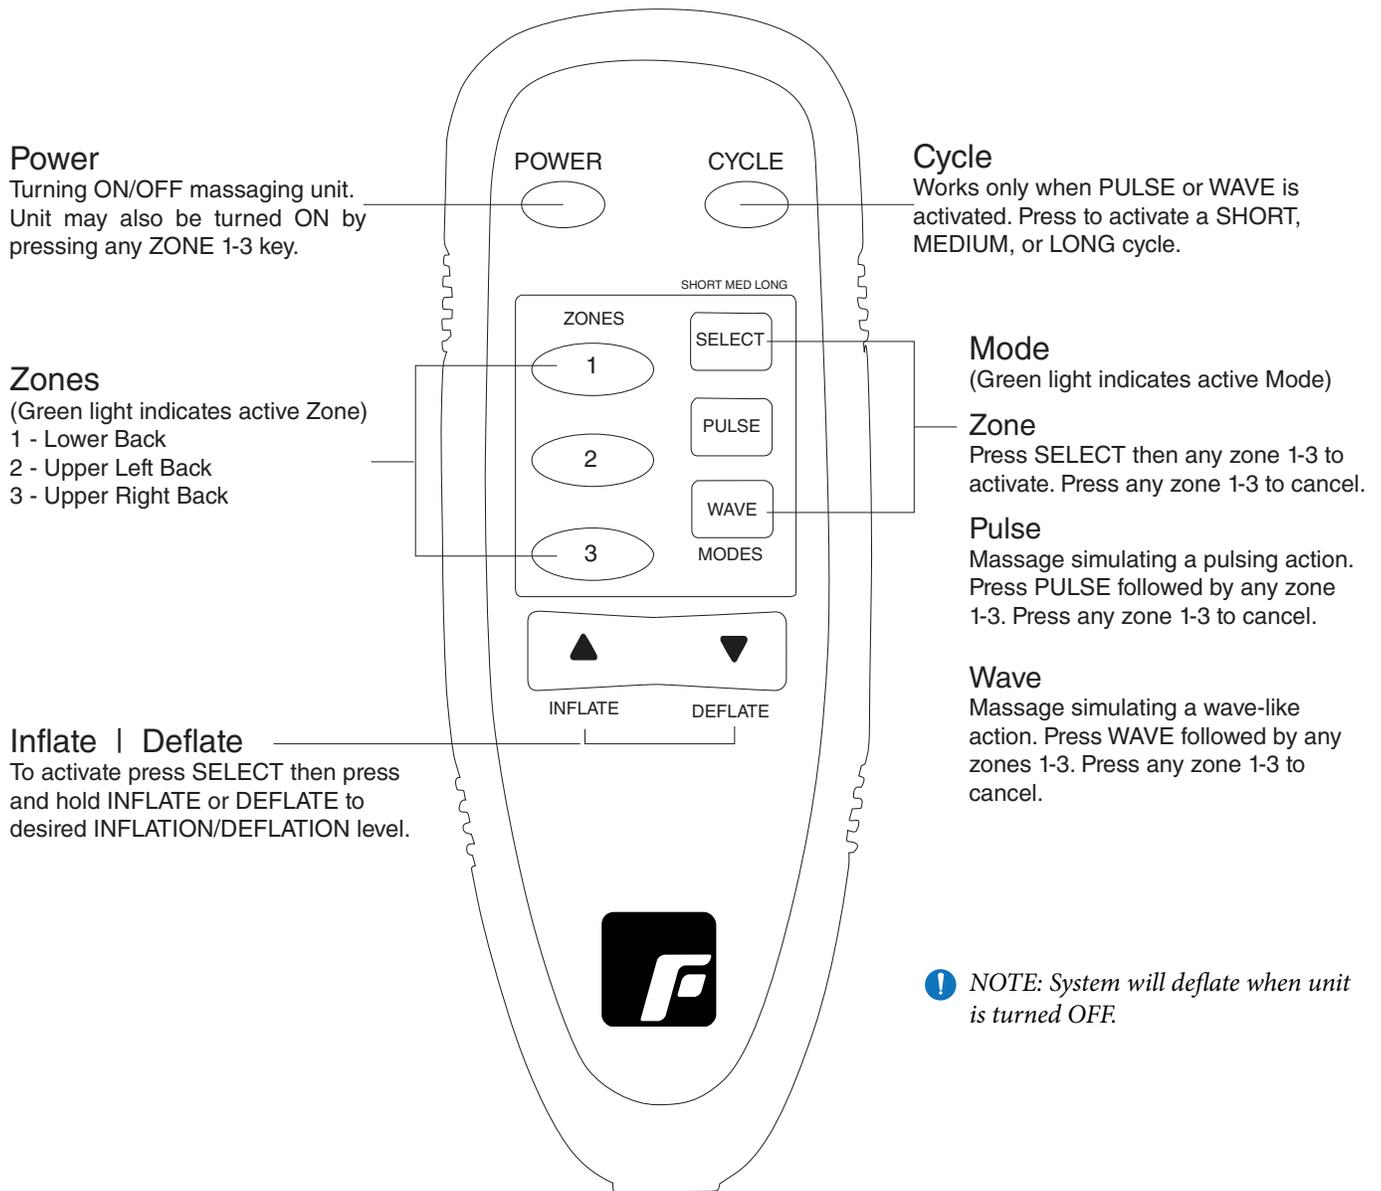

Forest Dental Equipment



DTE Oregon, Inc.
Address 6200 ne cherry drive hillsboro oregon 97124 • USA

Phone 800 . 423 . 3555 • 503 . 640 . 3012 | Fax 503 . 693 . 9715 | Digital sales@forestdental.com • forestdental.com



4.13.19 • 0097-345 • Rev. G • 2 of 2